

DEVELOPMENT SAMPLE DATA

This information is derived from development samples made available for evaluation. It does not necessarily imply that the device will go into regular production.

D12-120GH/109

INSTRUMENT CATHODE-RAY TUBE

12 cm diagonal rectangular flat-faced oscilloscope tube with mesh and metal-backed screen with internal graticule. The tube is intended for use in compact oscilloscopes.

QUICK REFERENCE DATA

Final accelerator voltage	$V_{g8(\ell)}$	10 kV
Display area		80 x 64 mm ²
Deflection coefficient		
horizontal	M_x	15,6 V/div
vertical	M_y	4,1 V/div

OPTICAL DATA

Screen		metal-backed phosphor
type		GH, colour green
persistence		medium short
Useful screen dimensions		$\geq 80 \times 64$ mm ²
Useful scan		
horizontal		≥ 80 mm
vertical		≥ 64 mm
Spot eccentricity in horizontal and vertical directions		$\leq 0,6$ div

HEATING

Indirect by a.c. or d.c.; parallel supply

Heater voltage	V_f	6,3 V
Heater current	I_f	95 mA

blue binder, tab 4



PHILIPS

June 1980

1

MECHANICAL DATA**Dimensions and connections**

See outline drawings

Overall length (socket included) ≤ 335 mmFace dimensions $\leq 88 \times 100$ mm²

Net mass approx. 700 g

Base 14 pin, all glass

Mounting position: any

The tube should not be supported by the base alone and under no circumstances should the socket be allowed to support the tube.

Accessories

Socket, supplied with tube type 55566

Side contact connector (5 required) type 55561

Final accelerator contact connector type 55563A

FOCUSING

electrostatic

DEFLECTION

double electrostatic

x-plates symmetrical

y-plates symmetrical

Angle between x and y-traces $90 \pm 1^\circ$ Angle between x-trace and x-axis of the internal graticule $\leq 5^\circ$ *

If use is made of the full deflection capabilities of the tube the deflection plates will block part of the electron beam, hence a low impedance deflection plate drive is desirable.

LIMITING VALUES (Absolute maximum rating system)

Final accelerator voltage	$V_{g8(\ell)}$	max. 11 kV min. 9 kV
Geometry control electrode voltage	V_{g7}	max. 2200 V
Post deflection shield and interplate shield voltage	V_{g6}	max. 2200 V
Deflection plate shield voltage	V_{g5}	max. 2200 V
Focusing electrode voltage	V_{g3}	max. 2200 V
First accelerator and astigmatism voltage	$V_{g2,g4}$	max. 2200 V min. 1350 V
Control grid voltage	V_{g1}	max. -200 V min. 0 V
Cathode to heater voltage		
positive	V_{kf}	max. 100 V
negative	$-V_{kf}$	max. 15 V
Voltage between astigmatism control electrode and any deflection plate	$V_{g4/x}$ $V_{g4/y}$	max. 500 V max. 500 V
Grid drive, average		max. 20 V
Screen dissipation	W_ℓ	max. 8 mW/cm ²
Control grid circuit resistance	R_{g1}	max. 1 M Ω

DEVELOPMENT SAMPLE DATA

* The tube is provided with a rotation coil, concentrically wound around the tube neck, enabling the alignment of the x-trace with the mechanical y-axis of the screen. Coil data to be fixed.

TYPICAL OPERATION

Conditions

Final accelerator voltage	$V_{g8(\ell)}$	10 kV
Geometry control electrode voltage	V_{g7}	1500 ± 100 V (note 1)
Post deflection shield and interplate shield voltage	V_{g6}	1500 V
Background illumination control voltage	ΔV_{g6}	0 to -15 V (note 1)
Deflection plate shield voltage	V_{g5}	1500 V (note 2)
Focusing electrode voltage	V_{g3}	250 to 350 V
First accelerator voltage	$V_{g2,g4}$	1500 V
Astigmatism control electrode voltage	$\Delta V_{g2,g4}$	± 50 V (note 3)
Control grid voltage for visual extinction of focused spot	V_{g1}	-20 to -60 V

Performance

Useful scan	horizontal	\geq	80 mm
	vertical	\geq	64 mm
Deflection coefficient	horizontal	M_x	\leq 15,6 V/div
	vertical	M_y	\leq 4,1 V/div
Line width			\leq 4,5 V/div
Grid drive for 10 μ A screen current	l.w.	typ.	0,35 mm (note 4)
Geometry distortion		approx.	12 V
Deviation of deflection linearity			see note 5
			$\leq 2\%$; see note 6

Notes

- The tube is designed for optimum performance when operating at a ratio $V_{g8(\ell)}/V_{g2,g4} = 6,7$. The geometry control electrode voltage V_{g7} should be adjusted within the indicated range (values with respect to the mean x-plate potential).
A negative control voltage V_{g6} (with respect to the mean x-plate potential) will cause some pincushion distortion and less background light, a positive control voltage will give some barrel distortion, and a slight increase of background light. By the use of the two voltages V_{g6} and V_{g7} , the best compromise between background light and raster distortion can be found.
- The deflection plate shield voltage should be equal to the mean y-plate potential. The mean x-plate and y-plate potentials should be equal for optimum spot quality.
- The astigmatism control electrode voltage should be adjusted for optimum spot shape. For any necessary adjustment its potential will be within the stated range.
- Measured with the shrinking raster method in the centre of the screen, under typical operating conditions, adjusted for optimum spot size, at a beam current of 10 μ A.
- A graticule consisting of concentric rectangles of 80 mm x 64 mm and 78,2 mm x 62,6 mm is aligned with the electrical x-axis of the tube. With optimum corrections applied, the edges of a raster will fall between these rectangles.
- The sensitivity at a deflection of less than 75% of the useful scan will not differ from the sensitivity at a deflection of 25% of the useful scan by more than the indicated value.

CAPACITANCES

x_1 to all other elements except x_2
 x_2 to all other elements except x_1
 y_1 to all other elements except y_2
 y_2 to all other elements except y_1
 x_1 to x_2
 y_1 to y_2
 Control grid to all other elements
 Cathode to all other elements

$C_{x1(x2)}$	5,3 pF
$C_{x2(x1)}$	5,3 pF
$C_{y1(y2)}$	3,6 pF
$C_{y2(y1)}$	3,6 pF
C_{x1x2}	2,1 pF
C_{y1y2}	1,7 pF
C_{g1}	5,5 pF
C_k	4,5 pF

DEVELOPMENT SAMPLE DATA



DIMENSIONS AND CONNECTIONS

Dimensions in mm

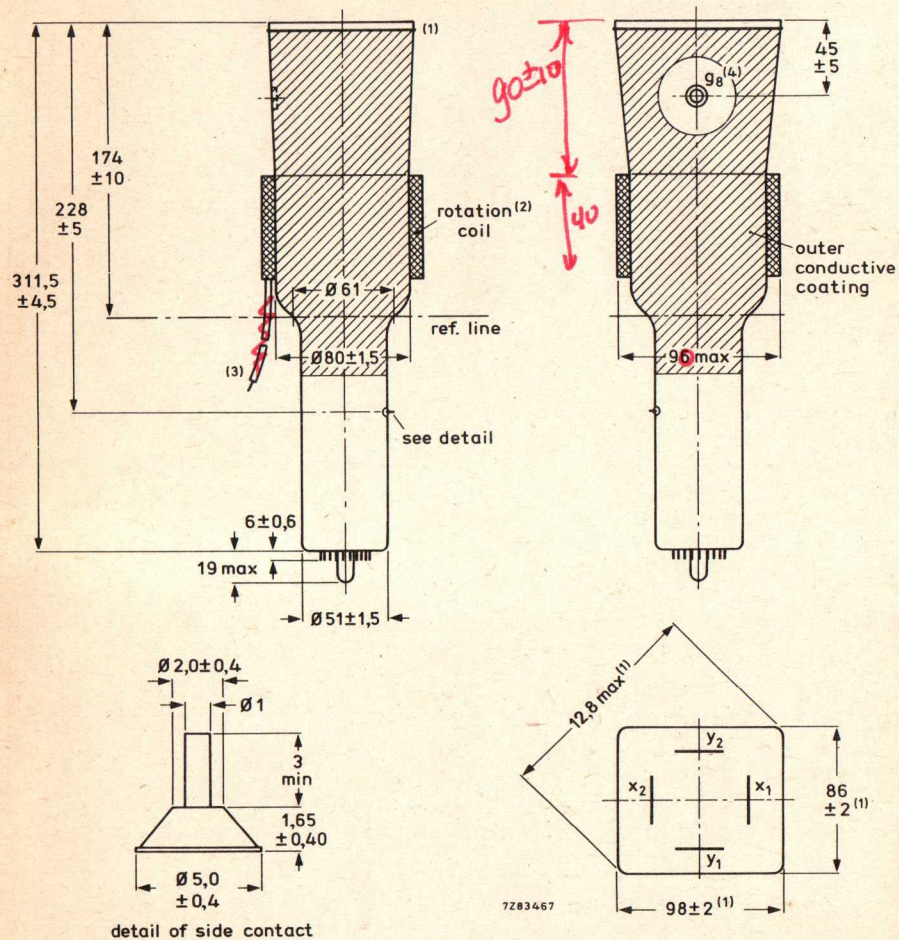


Fig. 1 Outlines; for notes see bottom of opposite page.

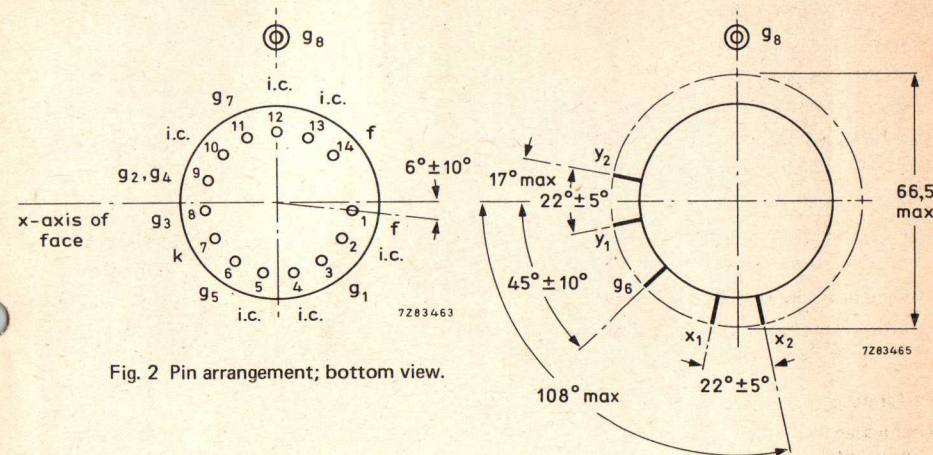


Fig. 2 Pin arrangement; bottom view.

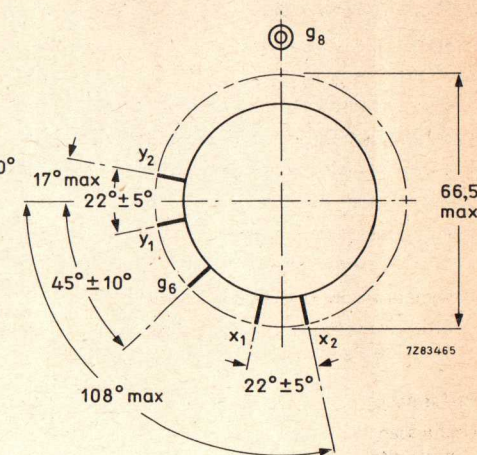


Fig. 3 Side-contact arrangement; bottom view.

DEVELOPMENT SAMPLE DATA

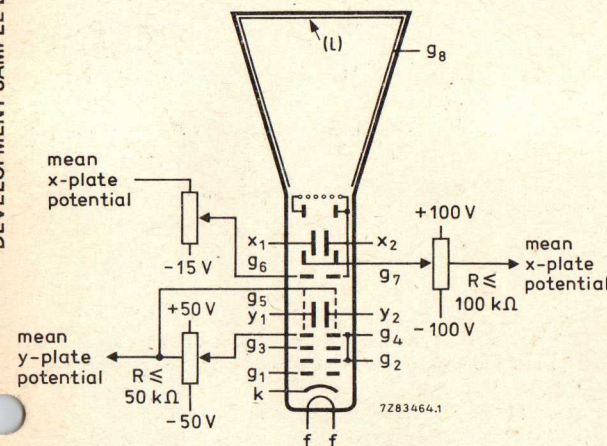


Fig. 4 Electrode configuration.




Fig. 5 Internal graticule. Line width = 0,18 mm; dot diameter = 0,36 mm.

Notes to the drawing on opposite page

1. The bulge at the frit seal may increase the indicated maximum dimensions by not more than 2,8 mm.
2. The coil is fixed to the envelope by means of adhesive tape.
3. Connection cable, comprising two wires for connection of the rotation coil, and one green wire for earthing the outer conductive coating. Minimum cable length is 350 mm.
4. The centre of the final accelerator contact is situated within a square of 10 mm x 10 mm around the true geometrical position.